



ODP8000 Series Programmable DC Power Supply User Manual

■ ODP8353

■ ODP8354

For product support, visit: www.owon.com.hk/download

※: The illustrations, interface, icons and characters in the user manual may be slightly different from the actual product. Please refer to the actual product.

Aug. 2025 edition V1.0.1

Copyright © LILLIPUT Company. All rights reserved.

The LILLIPUT's products are under the protection of the patent rights, including ones which have already obtained the patent rights and those which are applied for.

The information in this manual will replace all materials published.

The information in this manual was correct at the time of printing. However, LILLIPUT will continue to improve products and reserves the rights to change specification at any time without notice.

owon[®] is the registered trademark of the LILLIPUT Company.

Fujian LILLIPUT Optoelectronics Technology Co., Ltd.

No. 19, Heming Road

Lantian Industrial Zone, Zhangzhou 363005 P.R. China

Tel: +86-596-2130430

Fax: +86-596-2109272

Web: www.owon.com

E-mail: info@owon.com.cn

General Warranty

We warrant that the product will be free from defects in materials and workmanship for a period of 2 years from the date of purchase of the product by the original purchaser from our company. The warranty period for accessories is 12 months. This warranty only applies to the original purchaser and is not transferable to a third party.

If the product proves defective during the warranty period, we will either repair the defective product without charge for parts and labour, or will provide a replacement in exchange for the defective product. Parts, modules and replacement products used by our company for warranty work may be new or reconditioned like new. All replaced parts, modules and products become the property of our company.

To obtain service under this warranty, the customer must notify our company of the defect before the expiration of the warranty period. Customer shall be responsible for packaging and shipping the defective product to our designated service centre, a copy of the customer's proof of purchase is also required.

This warranty shall not apply to any defect, failure or damage caused by improper use or improper or inadequate maintenance and care. We shall not be obligated to furnish service under this warranty a) to repair damage resulting from attempts by personnel other than our company representatives to install, repair or service the product; b) to repair damage resulting from improper use or connection to incompatible equipment; c) to repair any damage or malfunction caused by the use of not our supplies; or d) to service a product that has been modified or integrated with other products when the effect of such modification or integration increases the time or difficulty of servicing the product.

Please contact the nearest sales and service offices for services.

Excepting the after-sales services provided in this summary or the applicable warranty statements, we will not offer any guarantee for maintenance definitely declared or hinted, including but not limited to the implied guarantee for marketability and special-purpose acceptability. We should not take any responsibilities for any indirect, special or consequent damages.

Table of Contents

1. General Safety Requirements	1
2. Safety Terms and Symbols	2
3. Quick Start	3
3.1 Front/Rear Panel and User Interface	3
3.1.1 Front Panel	3
3.1.2 Rear Panel	5
3.1.3 User Interface	6
3.2 General Inspection	7
3.3 Power-On Check	7
3.4 Output Inspection	7
3.4.1 Voltage Output Inspection	8
3.4.2 Current Output Inspection	8
4. Front Panel Operation	9
4.1 Turn On/Off the Channel Output	9
4.2 Set the Output Voltage/Current	9
4.2.1 Set the Output Voltage	9
4.2.2 Set the Output Current	10
4.3 Over Voltage/Current Protection	10
4.3.1 Set OVP	11
4.3.2 Set OCP	11
4.4 Save Settings/Auto Record	12
4.4.1 Manual Record	12
4.4.2 Auto Record	13
4.4.3 View Setting	13
4.4.4 View Record	13
4.5 Programmable Output	14
4.5.1 Data View	14
4.5.2 Output Set	15
4.5.3 Data process	15

4.6 Output mode	16
4.6.1 Independent Output	17
4.6.2 Parallel mode	17
4.6.3 Series mode	18
4.6.4 Channel track	19
4.6.5 Remote Compensation	20
4.7 Utility Settings	20
4.7.1 Language	20
4.7.2 Brightness	21
4.7.3 Beeper	21
4.7.4 Date	21
4.8 Port Settings	21
4.8.1 Serial Setting	21
4.8.2 LAN Setting	22
4.9 System Information	22
4.9.1 View System Information	22
4.9.2 Default Setting	23
4.9.3 Update	24
4.10 Other Settings	25
4.10.1 Knob Setting	25
4.10.2 Screen Test	26
4.10.3 Key Test	26
5. Troubleshooting	27
6. Technical Specification	28
ODP8353 Parameter	28
ODP8354 Parameter	31
General Parameter	33
7. Appendix	35
7.1 Appendix A: Packaging	35
7.2 Appendix B: General Care and Cleaning	35

1. General Safety Requirements

Before use, please read the following safety precautions to avoid any possible bodily injury and to prevent this product or any other connected products from damage. To avoid any contingent danger, ensure this product is only used within the ranges specified.

Only a qualified person should perform internal maintenance.

To avoid Fire or Personal Injury:

- **Use Proper Power Cord.** Use only the power cord supplied with the product and certified to use in your country.
- **Product Grounded.** This instrument is grounded through the power cord grounding conductor. To avoid electric shock, the grounding conductor must be grounded. The product must be grounded properly before any connection with its input or output terminals.
- **Check all Terminal Ratings.** To avoid fire or shock hazard, check all ratings and markings on this product. Refer to the user manual for more information about ratings before connecting to the instrument.
- **Do not operate without covers.** Do not operate the instrument with covers or panels removed.
- **Use the Proper Fuse.** Use only the specified type and rating fuse for this instrument.
- **Avoid exposed circuit.** Be careful when working on exposed circuitry to avoid risk of electric shock or other injury.
- **Do not operate if any damage.** If you suspect damage to the instrument, have it inspected by qualified service personnel before further use.
- **Use your instrument in a well-ventilated area.** Please keep well ventilated and inspect the intake and fan regularly.
- **Do not operate in damp conditions.** To avoid short circuiting to the interior of the device or electric shock, please do not operate in a humid environment.
- **Do not operate in an explosive atmosphere.** To avoid damages to the device or personal injuries, it is important to operate the device away from an explosive atmosphere.
- **Keep product surfaces clean and dry.** To avoid the influence of dust or moisture in air, please keep the surface of device clean and dry.

2. Safety Terms and Symbols

Safety Terms

Terms in this manual (The following terms may appear in this manual):



Warning: Warning indicates conditions or practices that could result in injury or loss of life.



Caution: Caution indicates the conditions or practices that could result in damage to this product or other property.

Terms on the product. The following terms may appear on this product:

Danger: Indicates an immediate hazard or injury possibility.

Warning: Indicates a possible hazard or injury.

Caution: Indicates potential damage to the instrument or other property.

Safety Symbols

Symbols on the product. The following symbols may appear on the product:



Hazardous Voltage



Refer to Manual



Protective Earth Terminal



Chassis Ground



Public Ground

3. Quick Start

3.1 Front/Rear Panel and User Interface

This manual uses the four-channel example for illustration. For the three-channel version, please refer to the four-channel instructions.

3.1.1 Front Panel

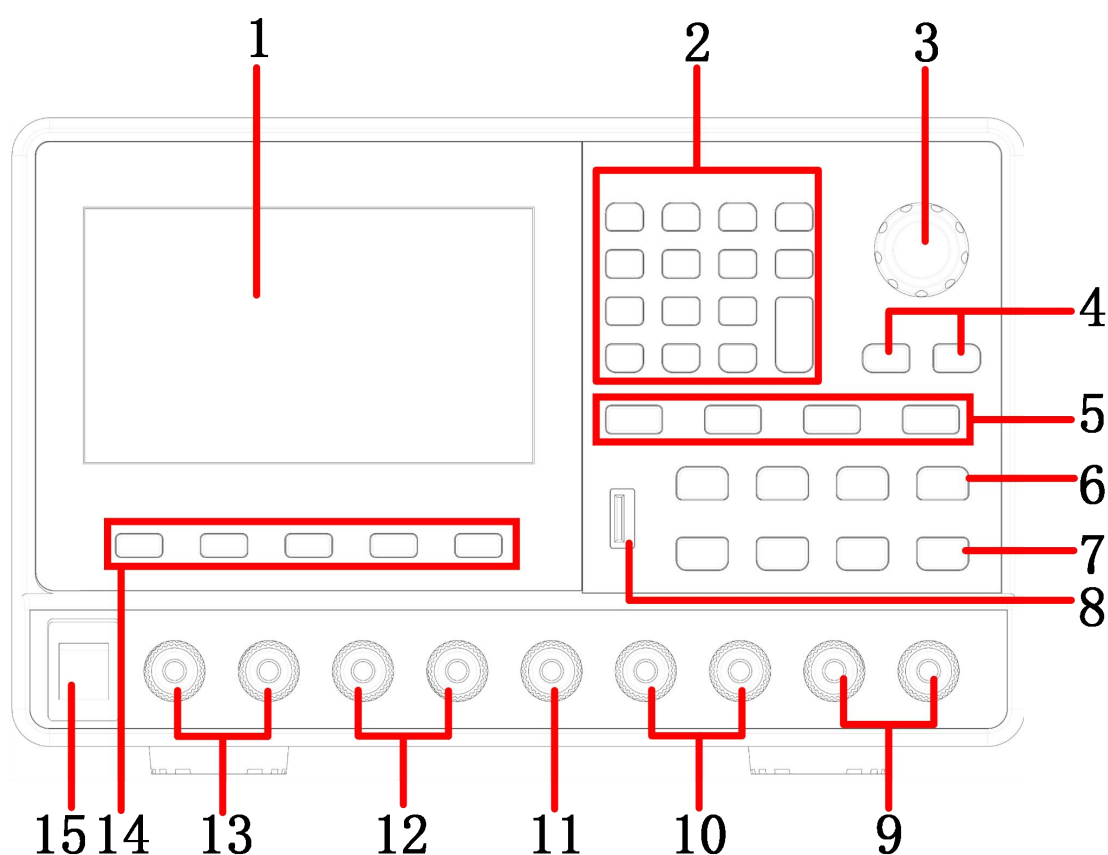


Figure 3- 1 Front panel overview

① LCD	User interface display.
② Numeric keys area	Parameter input, includes the numeric keys, decimal point and backspace key. Up and down direction key: Select sub menu. Enter key: Enter menu or confirm the parameter entered.

3.Quick Start

③ Knob	Select menu or change the value, pressing it has the same effect as pressing the enter key.
④ Left and right direction key	Set sub menu or move the cursor.
⑤ Function keys	Utility key: Menu of output mode, utility, info, port settings. Record key: Manual record, auto record, view setting and view recording. Program key: Programmable output. All On/Off key: Short press this key to enable/disable all channels output. Press and hold this key for 5 seconds to lock the panel keys. Unlock method: Press and hold the key for more than 5 seconds, and release.
⑥ Channel button	CH1, CH2, CH3, CH4 channel button, press it to select this channel.
⑦ On/Off button	Press the On/Off button of the corresponding channel to turn the channel output on or off.
⑧ USB Host port	Connect as a "host device" with an external USB device, such as connect a USB disk to the instrument.
⑨ CH4 output terminals	Channel 4 output connectors.
⑩ CH2 output terminals	Channel 2 output connectors.
⑪ Ground terminal	Channel ground connector.
⑫ CH1 output terminals	Channel 1 output connectors.

3.Quick Start

-
- | | | |
|---|-----------------------------|------------------------------|
| ⑬ | CH3 output terminals | Channel 3 output connectors. |
|---|-----------------------------|------------------------------|
-
- | | | |
|---|------------------------------|---|
| ⑭ | Menu selection button | Include 4 buttons, press it to select corresponding menu. |
|---|------------------------------|---|
-
- | | | |
|---|---------------------|----------------------------|
| ⑮ | Power button | Turn on/off the instrument |
|---|---------------------|----------------------------|
-

Instructions for panel key indicator

ON/OFF key: Press the button, and the channel light and the button light will turn on.

3.1.2 Rear Panel

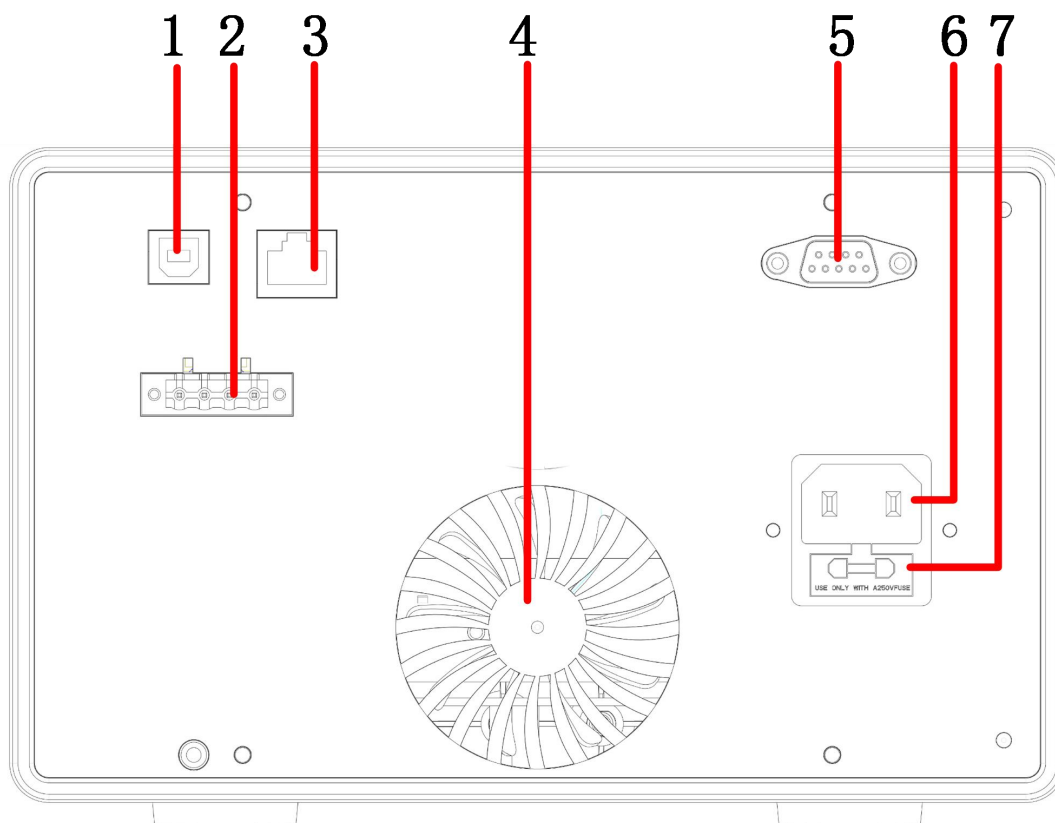


Figure 3-2 Rear panel overview

-
- | | | |
|---|-----------------------------|--|
| ① | USB Device Connector | Connect as a "slave device" with an external USB device, such as connect the instrument to a PC. |
|---|-----------------------------|--|
-
- | | | |
|---|----------------------------------|--|
| ② | S2+/S2-/S1+/S1- interface | Remote compensation voltage for Channel 1 and Channel 2, sample signal input port. |
|---|----------------------------------|--|
-

③	LAN interface	The power supply can be connected to the network for remote control via this connector.
④	Fan	Fan inlet.
⑤	RS232 interface	Serial port for connecting the instrument to external devices.
⑥	Power socket	AC input connector.
⑦	Fuse	Power supply fuse.

3.1.3 User Interface

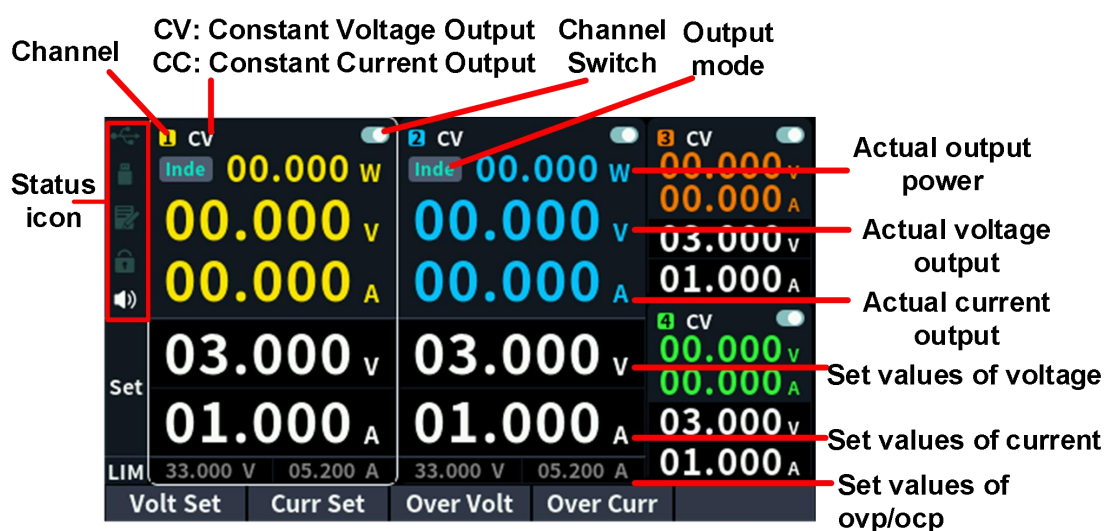


Figure 3-3 User interface in All channel mode

Status Icons

Icons	Instruction
	USB Communication Port Priority
	USB Device Priority
	Recording the current output
	The panel keys are locked
	The beeper is turned on

3.2 General Inspection

When you receive your new power supply, it is recommended that you check the instrument following these steps:

1. Check for transportation damage.

If it is found that the packaging carton or the foamed plastic protection cushion has suffered serious damage, do not throw it away first till the complete device and its accessories succeed in the electrical and mechanical property tests.

2. Check the Accessories

The supplied accessories are described in the "Appendix A: " of this Manual. You can check whether there is any loss of accessories with reference to this description. If it is found that there is any accessory lost or damaged, please get in touch with the distributor of our responsible for this service or our local offices.

3. Check the Complete Instrument

If it is found that there is damage to the appearance of the instrument, or the instrument can not work normally, or fails in the performance test, please get in touch with our distributor responsible for this business or our local offices. If there is damage to the instrument caused by the transportation, please keep the package. With the transportation department or our distributor responsible for this business informed about it, a repairing or replacement of the instrument will be arranged by us.

3.3 Power-On Check

- (1) Connect the instrument to the AC supply using the supplied power cord.



Warning:

To avoid electric shock, the instrument must be grounded properly.

- (2) Push the **power button** on the front panel, the screen will show the startup screen.

3.4 Output Inspection

Output inspection is to ensure that the instrument can achieve its rated outputs

and properly respond to operation from the front panel. For the procedures below, it is suggested that you read "*Turn On/Off the Channel Output*" on page 9 and "*Set the Output Voltage/Current*" on page 9.

3.4.1 Voltage Output Inspection

The following steps verify basic voltage functions without load:

- (1) When the instrument is under no load, select a channel and ensure the output current setting for this channel is not at zero.
- (2) Turn on the channel output, then ensure the channel is in Constant Voltage output mode.
- (3) Set some different voltage values on this channel; check if the actual voltage value displayed is close to the set voltage value, and also that the actual current value displayed is nearly to zero.
- (4) Check that if the output voltage can be adjusted from zero to the maximum rating.

3.4.2 Current Output Inspection

The following steps check basic current functions with a short across the power supply's output:

- (1) Connect a short across (+) and (-) output terminals with an insulated test lead on this channel. Use a wire size sufficient to handle the maximum current.
- (2) Set the output voltage to the maximum rating on this channel.
- (3) Turn on the channel output. Ensure the channel you used is in Constant Current output mode.
- (4) Set some different current values on this channel; check if the actual current value displayed is close to the set current value, and to check if the actual voltage value displayed is nearly zero.
- (5) Check that if the output current can be adjusted from zero to the maximum rating.
- (6) Turn off the channel output and remove the short circuit from the output terminals.

4. Front Panel Operation

4.1 Turn On/Off the Channel Output

Yellow **On/Off** button: Pressing the **On/Off** button will turn on the output of Channel 1, and the button light will turn on. Pressing the button again will turn off the output of Channel 1, and the button light will turn off.

Blue **On/Off** button: Pressing the **On/Off** button will turn on the output of Channel 2, and the button light will turn on. Pressing the button again will turn off the output of Channel 2, and the button light will turn off.

Orange **On/Off** button: Pressing the **On/Off** button will turn on the output of Channel 3, and the button light will turn on. Pressing the button again will turn off the output of Channel 3, and the button light will turn off.

Green **On/Off** button: Pressing the **On/Off** button will turn on the output of Channel 4, and the button light will turn on. Pressing the button again will turn off the output of Channel 4, and the button light will turn off.

4.2 Set the Output Voltage/Current

4.2.1 Set the Output Voltage

- **Set the output voltage of CH1**

Press the **CH1** button to select Channel 1, then press the **Volt Set** key, CH1 set voltage is flashing, indicating the value is editable. The following methods can be used to set the value:

- Turn the **knob** to change the value. Press the  /  key to move the cursor. Press the  key to confirm.
- Use the **numeric keys** to input, the input box of **Channel 1** output voltage will pop up. Enter a desired value. Press the  key to confirm.

- **Set the output voltage of CH2**

Press the **CH2** button to select Channel 2, then press the **Volt Set** key to enter edit mode. You can set the value in the same way as CH1 above.

- **Set the output voltage of CH3**

Press the **CH3** button to select Channel 3, then press the **Volt Set** key to enter edit mode. You can set the value in the same way as CH1 above.

- **Set the output voltage of CH4**

Press the **CH4** button to select Channel 4, then press the **Volt Set** key to enter edit mode. You can set the value in the same way as CH1 above.

4.2.2 Set the Output Current

- **Set the output current of CH1**

Press the **CH1** button to select Channel 1, then press the **Curr Set** key, CH1 set current is flashing, indicating the value is editable. The following methods can be used to set the value:

- Turn the **knob** to change the value. Press the  /  key to move the cursor. Press the  key to confirm.
- Use the **numeric keys** to input, the input box of **Channel 1** output current will pop up. Enter a desired value. Press the  key to confirm.

- **Set the output current of CH2**

Press the **CH2** button to select Channel 2, then press the **Curr Set** key to enter edit mode. You can set the value in the same way as CH1 above.

- **Set the output current of CH3**

Press the **CH3** button to select Channel 3, then press the **Curr Set** key to enter edit mode. You can set the value in the same way as CH1 above.

- **Set the output current of CH4**

Press the **CH4** button to select Channel 4, then press the **Curr Set** key to enter edit mode. You can set the value in the same way as CH1 above.

Note: If the input value is out of the rated range, the box prompts "Over The Limit!"; you need to input another value within the rated range.

4.3 Over Voltage/Current Protection

When the Over Voltage Protection or Over Current Protection is enabled, once the output voltage/current reaches the set value, the instrument will cut off the output,

a warning will show on the screen.

Note:

When the instrument disables the output due to protection, after you make some adjustments, the channel must be restarted to output normally.

This function can keep the power output from exceeding the load rating to protect the load.

4.3.1 Set OVP

- **Set the OVP of CH1**

Press the **CH1** button to select Channel 1, then press the **Over Volt** key, CH1 set OVP is flashing, indicating the value is editable. The following methods can be used to set the value:

- Turn the **knob** to change the value. Press the **< / >** key to move the cursor. Press the  key to confirm.
- Use the **numeric keys** to input, the input box of **Channel 1** output OVP will pop up. Enter a desired value. Press the  key to confirm.

- **Set the OVP of CH2**

Press the **CH2** button to select Channel 2, then press the **Over Volt** key to enter edit mode. You can set the value in the same way as CH1 above.

- **Set the OVP of CH3**

Press the **CH3** button to select Channel 3, then press the **Over Volt** key to enter edit mode. You can set the value in the same way as CH1 above.

- **Set the OVP of CH4**

Press the **CH4** button to select Channel 4, then press the **Over Volt** key to enter edit mode. You can set the value in the same way as CH1 above.

4.3.2 Set OCP

- **Set the OCP of CH1**

Press the **CH1** button to select Channel 1, then press the **Over Curr** key, CH1

set OCP is flashing, indicating the value is editable. The following methods can be used to set the value:

- Turn the **knob** to change the value. Press the  /  key to move the cursor. Press the  key to confirm.
- Use the **numeric keys** to input, the input box of **Channel 1** output OCP will pop up. Enter a desired value. Press the  key to confirm.

- **Set the OCP of CH2**

Press the  button to select Channel 2, then press the  key to enter edit mode. You can set the value in the same way as CH1 above.

- **Set the OCP of CH3**

Press the  button to select Channel 3, then press the  key to enter edit mode. You can set the value in the same way as CH1 above.

- **Set the OCP of CH4**

Press the  button to select Channel 4, then press the  key to enter edit mode. You can set the value in the same way as CH1 above.

4.4 Save Settings/Auto Record

4.4.1 Manual Record

Press the  key. Then press  to enter manual record menu. You can save, recall and delete current setting parameters. The storage memory could be set as internal or USB flash device. Up to 100 groups of settings can be saved.

- (1) Press  /  to select **Save**, then Press the  /  key to the channel (CH1, CH2), press the  key to save the setting of the selected channel.
- (2) Press  /  to select **Delete**, then rotary the knob to select the item which you desired to delete. Press the  /  key to turn the page. Press the  key to delete.
- (3) Press  /  to select **Recall**, then rotary the knob to select the item. Press the  /  key to turn the page. Press the  key to recall.

4.4.2 Auto Record

Press the **Record** key. Then press **Auto** to enter automatic record menu.

- (1) Press  /  to select **Interval**. Use the **numeric keys** to set the record interval, press the  key to confirm.
- (2) Press  /  to select **Points**. Use the **numeric keys** to set the points, press the  key to confirm.
- (3) Press  /  to select **Channel**. Press the  /  key to the channel (CH1, CH2), press the  key to save the setting of the selected channel.
- (4) Press  /  to select **Record**. Press the  key to start recording the output of the selected channel. Press the  key again to stop recording.

During recording, the icon  will be lighted on the status bar.

4.4.3 View Setting

Press the **Record** key. Then press **View Set** to enter view setting menu. Only records in the internal storage source can be viewed; records from the internal storage source can be exported to an external storage source.

- (1) Press  /  to select **Channel**. Press the  /  key to the channel (CH1, CH2), press the  key to save the setting of the selected channel.
- (2) Press  /  to select **Display**. Press the  /  key to select **Sheet** or **Wave**.
- (3) Press  /  to select **Export**. Then insert U disk, press the  key to export the recording file of the selected channel onto the U disk. The directory is **ODPXXXX\Record** (ODPXXXX is the model).
- (4) Press  /  to select **Clear**. Press the  key to clear the recording file.

4.4.4 View Record

Press the **Record** key. Then press **View** to enter view record menu. Press the  /  key to turn the page.


4.Front Panel Operation

If the display mode is set to Sheet, the records will be displayed in table format; if the display mode is set to Wave, the records will be displayed in waveform format.

NO	CH1		
	Volt	Curr	Power
1	04.000	01.170	04.680
2	04.000	01.170	04.680
3	04.000	01.170	04.680
4	04.000	01.170	04.680
5	04.000	01.170	04.680
6	04.000	01.170	04.680
7	08.000	01.170	09.360
8	08.000	01.170	09.360
9	08.000	01.170	09.360
10	08.000	01.190	09.520

Manual Auto View Set View

Sheet display mode

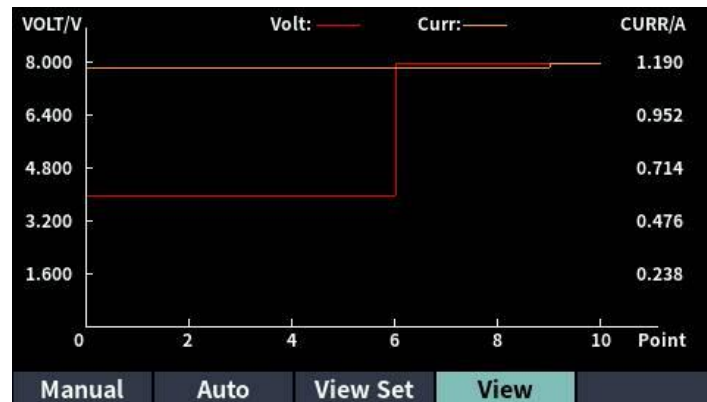

Wave display mode

4.5 Programmable Output

The programmable output function can preset up to 100 groups of timing parameters. When you turn on the programmable output, the instrument will output the pre-specified voltage, current in pre-specified time.

4.5.1 Data View

Press the **Program** key. Then press **Data** to enter data view menu.

- (1) Press **▲** / **▼** to select **Import**. Insert U disk and press the **↵** key to import data.

Note: The exported file can be edited using Excel. After editing, remove "xx_xx_xx_Export" from the file name. The import file format should be

Program_XXXXXXXX.csv, where XXXXXXXXX represents the serial number.

The file must be placed in the Program subfolder to be recognized.

- (2) Press  /  to select **Export**. Insert U disk and press the  key to export data.

Note: The programming data file will be saved in CSV format to the USB drive, with the storage path under the Program subfolder in the USB storage device folder named XXXXXXXXX_xx_xx_xx_Export (model name).

- (3) Press  /  to select **Clear**. Press the  key to clear data.

4.5.2 Output Set

The output settings allow you to define the start point, end point, and output method for programmed output. During programmed output, the system will follow the settings to sequentially or cyclically output the preset parameters between the start point and the end point.

Press the **Program** key. Then press **Output** to enter output setting menu.

- (1) Press  /  to select **Cycle**. Press the  /  key to select **Oder** or **Loop**.

- (2) Press  /  to select **Range**. Press the  /  key to select **Begin** or **End**.

Use the **numeric keys** to input (1 to 100), press the  key to confirm.

- (3) Press  /  to select **Channel**. Press the  /  key to the channel (CH1, CH2 or All), press the  key to save the setting of the selected channel.

- (4) Press  /  to select **Output**. Press the  key to confirm output. Press the  key to return to the submenu selection.

4.5.3 Data process

You can set the programmable parameters of CH1 and CH2, including voltage, current and output time. This function allows up to 100 parameter groups of each channel.

Press the **Program** key. Then press **Edit** to enter data edit menu.

(1) In the data processing interface, Press the  /  key to turn the page.

Press the  /  key to move the cursor up and down. Turn the knob to move the cursor between CH1 and CH2. Use the After selecting the parameter, use the numeric keys to enter a desired value, press the  key to confirm.

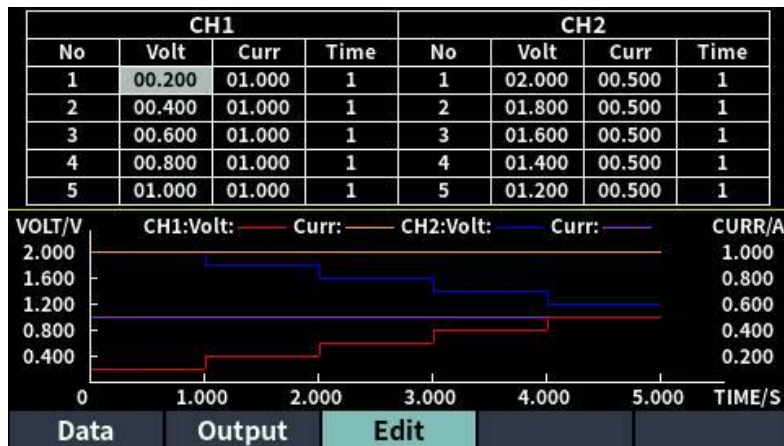


Figure 4- 1 Data processing Interface

4.6 Output mode

Output mode can simplify the parameter inputting of CH1 and CH2. Output mode setting is only for CH1 and CH2, without affecting CH3. There are four output modes.

To set the output mode:

- (1) Press the **Utility** key. Then press **Mode** to enter output mode menu.
- (2) Press the  /  key to select the **Output**. Press the  /  key to choose **Independ**, **Series**, **Parallel** or **Track** as current output mode.
- (3) Press the  /  key to select the **Sense**. Press the  /  key to choose **OFF** or **ON** to enable or disable remote compensation function.
- (4) Press the  /  key to select the **Device**. Press the  /  key to choose **USBTMC** or **Udisk**. When performing USBTMC communication, select USBTMC. When you need to upgrade through a USB flash drive, select Udisk.

4.6.1 Independent Output


The parameter of each channel can be set independently.



4.6.2 Parallel mode


When CH1 and CH2 are connected in parallel, you can select this mode to simplify the parameter inputting. You just need to set the parameters of the combined channel.

Press the **yellow/blue On/Off** key to turn on/off the combined channel.

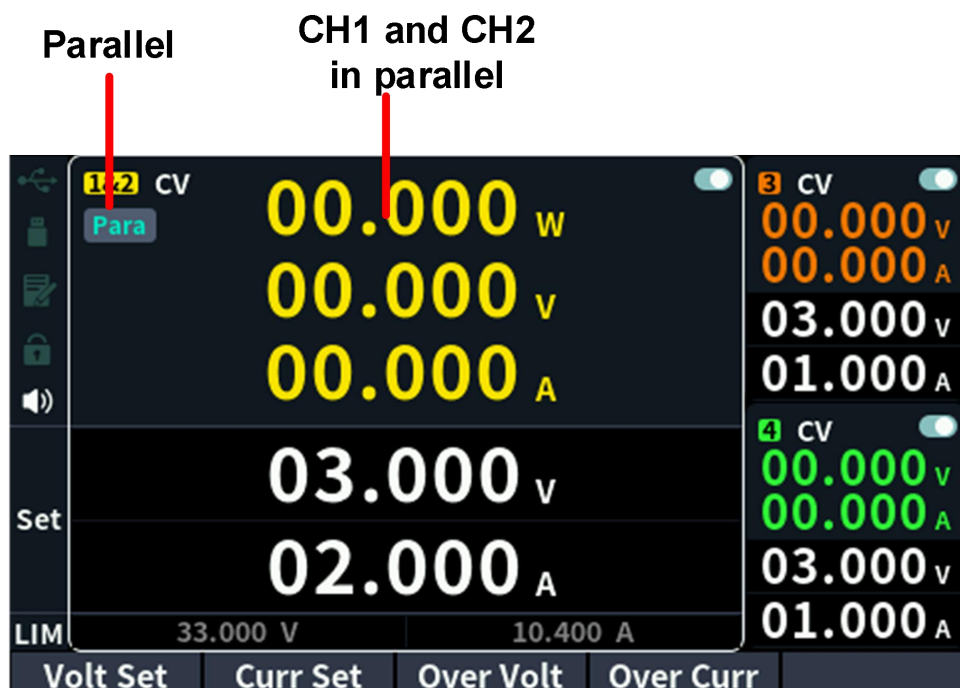

4. Front Panel Operation


The connection method of the parallel connection of CH1 and CH2 is as shown in the figure below.

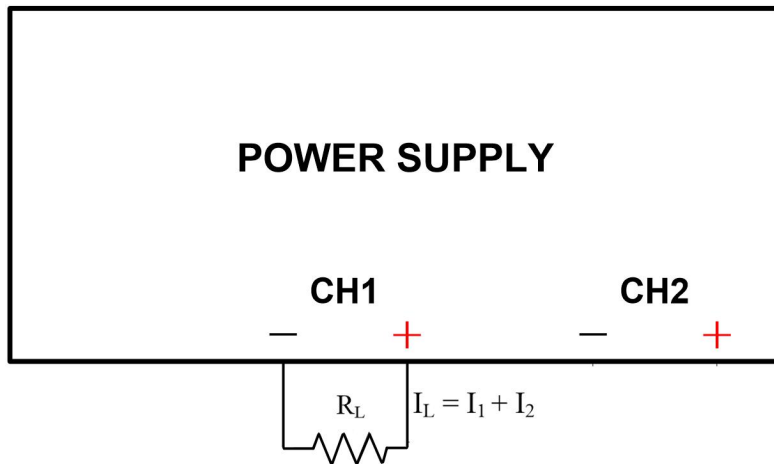


4.6.3 Series mode

When CH1 and CH2 are connected in series, you can select this mode to simplify the parameter inputting. You just need to set the parameters of the combined channel.

Press the **orange On/Off** key to turn on/off the combined channel.

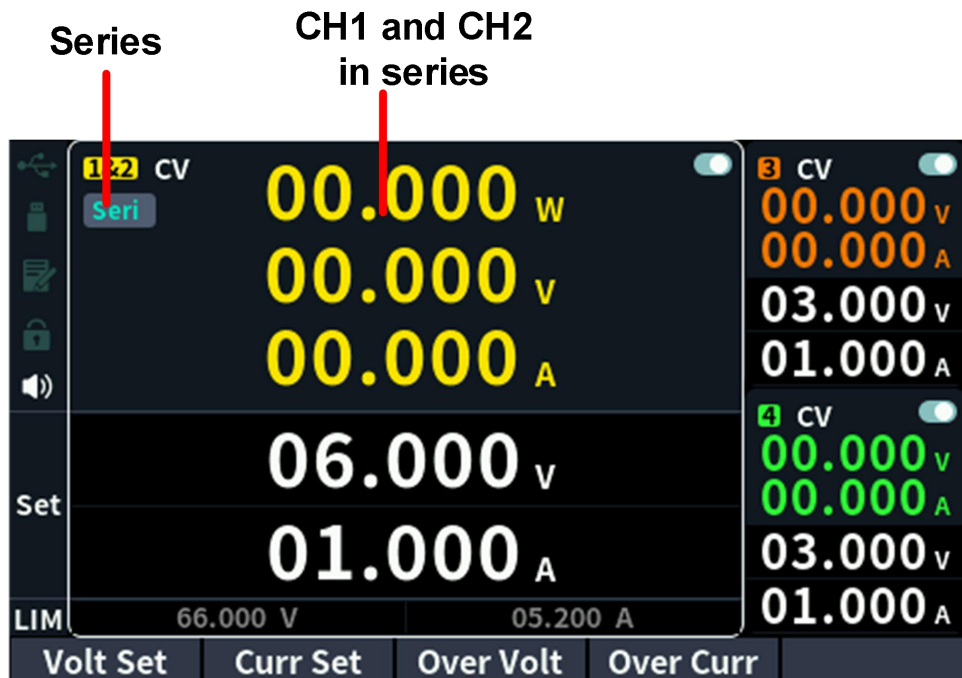

The connection method of the series connection of CH1 and CH2 is as shown in the figure below.

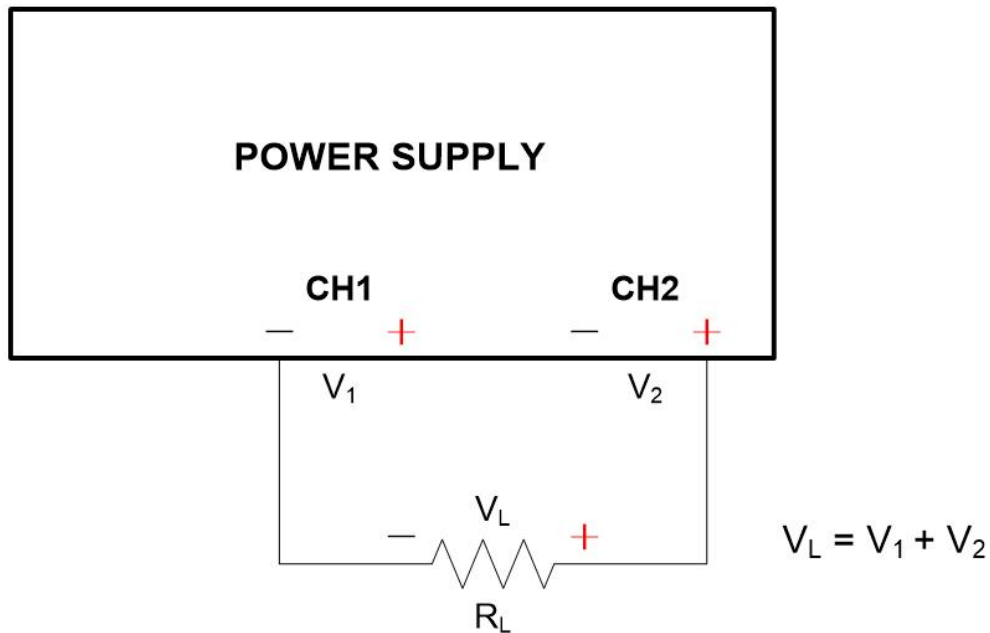


4.6.4 Channel track

When users need both Channel 1 and Channel 2 to output the same voltage and current simultaneously, they can enter the Channel Tracking mode. In this mode, identical voltage and current parameters can be set for both channels simultaneously.

Note: If the setting value is out of the rated range, it will be set to the maximum.


Channel 1 track

Channel 2 track

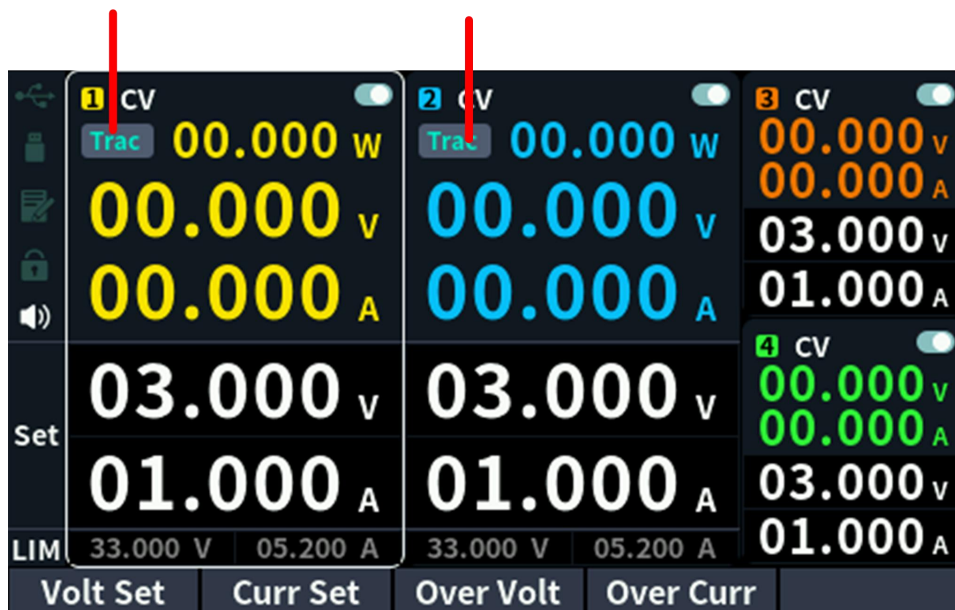

4.6.5 Remote Compensation

Please connect the wires as shown in the following diagram after enabling the remote compensation function.

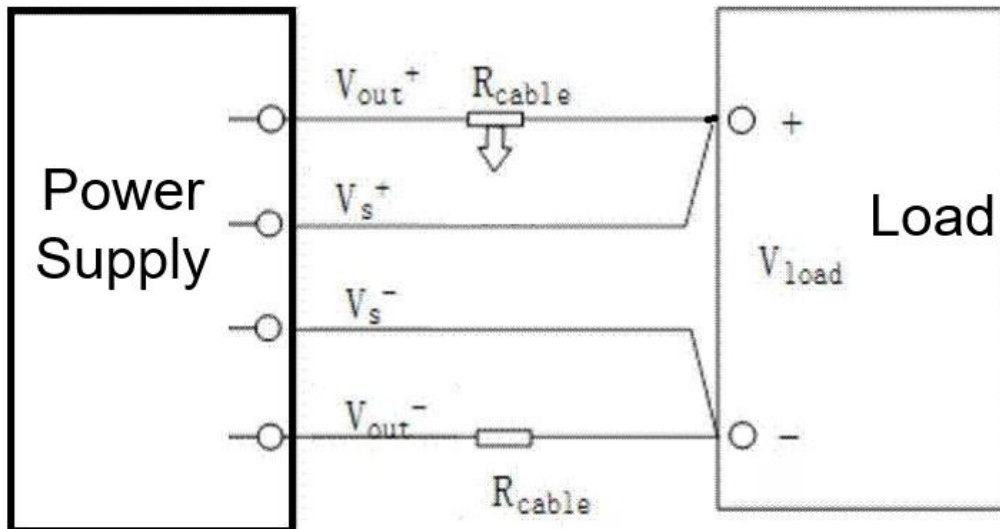

Note:

- Please strictly follow the wiring diagram when connecting, and only start the power supply after confirming the connections are correct.
- Always turn off the power output before disconnecting any cables when you finish using the power supply.
- For the safety of power equipment, the maximum compensation voltage for remote compensation shall not exceed 1V. It is recommended to use 16AWG or 1.5mm² copper conductors for the connection wires of power output terminals.

4.7 Utility Settings

4.7.1 Language

- (1) Press the **Utility** key. Then press **System** to enter system setting menu.
- (2) Press the **▲** / **▼** key to select the **Language**. Press the **<** / **>** key to choose the desired language. The supported languages include: Chinese, English and so on.

4.7.2 Brightness

- (1) Press the **Utility** key. Then press **System** to enter system setting menu.
- (2) Press the  /  key to select the **Screen**. Use the knob or numeric keypad to set the desired value.

4.7.3 Beeper

- (1) Press the **Utility** key. Then press **System** to enter system setting menu.
- (2) Press the  /  key to select the **Buzzer**. Press the  /  key to turn on/off the beeper. When the beeper is on, the icon  will be lighted on the status bar. When the system prompts the instrument will make a buzzing sound, e.g. cutting off the output due to OVP/OCP.

4.7.4 Date

- (1) Press the **Utility** key. Then press **System** to enter system setting menu.
- (2) Press the  /  key to select the **Date**. Press the  /  key to move the cursor. Use the knob or numeric keypad to set the desired value, press the  key to confirm.

4.8 Port Settings

4.8.1 Serial Setting

- (1) Press the **Utility** key. Then press **Interface** to enter interface setting menu.
- (2) Press the **Interface** key to select the **Serial**.
- (3) Press the  /  key to select **Baudrate**. Press the  /  key to select the desired baud rate from 1200, 2400, 4800, 9600, 19200, 38400, 57600 or 115200. The default is 115200. Make sure that the baud rate matches that of the computer.
- (4) Press the  /  key to select **Data Bits**. Press the  /  key to select 6, 7, or 8.
- (5) Press the  /  key to select **Stop Bits**. Press the  /  key to 1 or 2.

- (6) Press the  /  key to select **Parity**. Press the  /  key to select None, Odd, or Even.

4.8.2 LAN Setting

- (1) Press the **Utility** key. Then press **Interface** to enter interface setting menu.
- (2) Press the **Interface** key to select the **Lan**.
- (3) Press the  /  key to select the **IP Address**. Press the  /  key to move the cursor. Use the knob or numeric keypad to set the desired value, press the  key to confirm.
- (4) Press the  /  key to select the **Net Mask**. Press the  /  key to move the cursor. Use the knob or numeric keypad to set the desired value, press the  key to confirm.
- (5) Press the  /  key to select the **Gateway**. Press the  /  key to move the cursor. Use the knob or numeric keypad to set the desired value, press the  key to confirm.
- (6) Press the  /  key to select the **Port**. Press the  /  key to move the cursor. Use the knob or numeric keypad to set the desired value, press the  key to confirm.
- (7) Press the  /  key to select the **DHCP**. Press the  /  key to enable or disable DHCP function. You can manually adjust IP information only when DHCP function is disabled.

Note: Restart the instrument for the parameter changes to take effect.

4.9 System Information

4.9.1 View System Information

- (1) Press the **Utility** key. Then press **Info** to enter system information menu.
- (2) Press the  /  key to select the **Info**. You can view the version, series number, checksum and so on.

4.9.2 Default Setting

(1) Press the **Utility** key. Then press **Info** to enter system information menu.

(2) Press the  /  key to select the **Default**. Press the  key to use the factory defaults, see table below.

Output Setting	Output		VOLT	CURR	
	CH1		03.000V	01.000A	
	CH2				
	CH3				
	CH4				
	Parallel		03.000V	02.000A	
	Series		06.000V	01.000A	
Limit Setting	Output		VOLT	CURR	
	CH1		32.000V	05.200A	
	CH2				
	CH3		25.000V	03.200A	
	CH4				
	Parallel		32.000V	10.400A	
	Series		64.000V	05.200A	
Utility	Output		Independent		
	Sense		OFF		
	Screen		50%		
	Buzzer		ON		
	Interface setting	Series	Baudrate		115200
			Data Bits		8
			Stop Bits		1
			Parity		None
		Lan	IP		192.168.000.001
			Net Mask		255.255.255.000
			Gateway		192.168.001.254

4.Front Panel Operation

			Port	3000
Record	Save	Channel	CH1	
	Auto	Interval	1	
		Points	1000	
		Channel	CH1	
	View	Channel	CH1	
		Display	Sheet	
Program	Output	Cycle	Order	
		Range	Begin: 1 ~ End: 100	
		Channel	CH1	

4.9.3 Update

Use the front-panel USB port to update your instrument firmware using a USB memory device.

USB memory device requirements: This instrument only supports a USB memory device with a FAT32 file system. If the USB memory device doesn't work properly, format it into the FAT32 format and try again; or try another USB memory device.



Caution: Updating your instrument firmware is a sensitive operation, to prevent damage to the instrument, do not power off the instrument or remove the USB memory device during the update process.

To update your instrument firmware, do the following:

- (1) Press the **Utility** key. Then press **Info** to enter system information menu.
- (2) Press the **▲** / **▼** key to select the **Info**. You can view the model and firmware version.
- (3) From a PC, visit our website and check if the website offers a newer firmware version. Download the firmware file. The file name must be ODP.upp. Copy the firmware file onto the root directory of your USB memory device.
- (4) Insert the USB memory device into the front-panel USB port on your

instrument. If the status icon  appears on the left of the screen, the USB memory device is installed successfully.

(5) Press the  /  key to select the **Update**. Press the  key to start update.

(6) The instrument displays a message telling you not to remove the USB device or power off the instrument until the update process is complete. The progress bar of the screen indicates the update process is in progress.

Note: A firmware update usually takes approximately a minute. Do not remove the USB memory device during the update process. If you accidentally removed the USB memory device during the update process, do not power off the instrument. Repeat the installation process from step 3.

(7) Wait until the instrument displays "Firmware upgrade success.", and then it will reboot automatically.

Note: If the operation complete message is not displayed, do not power off the instrument. Repeat the installation process from step 3 using a different type of USB memory device.

(8) Remove the USB memory device from the front-panel USB connector.

(9) Press the **Utility** key. Then press **Info** to enter system information menu. Press the  /  key to select the **Info**, view the firmware version. Confirm that the firmware has been updated.

4.10 Other Settings

4.10.1 Knob Setting

Output mode when setting the output value by rotating the knob.

(1) Press the **Utility** key. Then press **Other** to enter other setting menu.

(2) Press the  /  key to select the **Knob**. Press the  /  key to select

After press Enter or Directly output.

4.10.2 Screen Test

The instrument has a screen self test function, which can test the LCD screen.

- (1) Press the **Utility** key. Then press **Other** to enter other setting menu.
- (2) Press the  /  key to select the **Screen**. Press the  key to enter the screen test interface. Observe if the screen has severe color shift, spot, scuffing, or other defect.
- (3) Press the  key to exit the test.

4.10.3 Key Test

The instrument provides the key self testing, which can test the keys on the front panel.

- (1) Press the **Utility** key. Then press **Other** to enter other setting menu.
- (2) Press the  /  key to select the **Key**. Press the  key to enter the key test interface. Each shape on the test interface represents a front panel key. Press any front panel key, the corresponding shape on the test interface will turn green.
- (3) Press the  key to exit the test.

5. Troubleshooting

1. The instrument is powered on but no Display.

- Check if the power is connected properly.
- Check if the fuse which is below the AC Power socket is used appropriately and in good condition (the cover can be pried open with a straight screwdriver).
- Restart the instrument after the steps above.

2. The output is abnormal:

- Check if the output voltage is set to 0V. If so, set it to other value.
- Check if the output current is set to 0A. If so, set it to other value.
- When in programmable output status, check if there is any voltage/current value is set to 0. If so, set it to other value.

3. Cannot identify the USB device correctly:

- Check if the system settings prioritize USB devices. If you want to use a USB flash drive, set USB devices as the priority.
- Check if the USB device is in good condition.
- Check if the used USB device is a flash device, note a hard disk cannot be supported.

4. USB cannot communication:

- Check if USB communication is prioritized in the system settings. If you want to use USB communication, set USB communication as the priority.

Check if the used USB device is a flash device, note a hard disk cannot be

If you encounter any other issues, please try restarting. If the product still does not function properly, please contact us so we can assist you.

6. Technical Specification

The specifications below are based on the instrument having run for at least 30 minutes continuously under the specified operating temperature.

ODP8353 Parameter

Parameter		Description	
Output Ratings (0°C-40°C)	Voltage/ Current	CH1: 32V/5A, Maximum 102W constant power output	
		CH2: 32V/5A, Maximum 102W constant power output	
		CH3: 24V/3A, Maximum 24W constant power output	
	CH1,CH2 Parallel Voltage/ Current	64V/5A, Maximum 204W constant power output	
	CH1,CH2 Series Voltage/ Current	32V/10A, Maximum 204W constant power output	
Channel		3	
Load Regulation	Independent	Voltage	$\leq 0.01\% + 5\text{mV}$
	Parallel	Voltage	$\leq 0.01\% + 50\text{mV}$
	Series	Voltage	$\leq 0.01\% + 50\text{mV}$
Voltage Regulation	Independent	Voltage	$\leq 0.01\% + 3\text{mV}$
		Current	$\leq 0.01\% + 3\text{mA}$
	Parallel	Voltage	$\leq 0.01\% + 3\text{mV}$
		Current	$\leq 0.01\% + 3\text{mA}$

6. Technical Specification

	Series	Voltage	$\leq 0.01\% + 3\text{mV}$
		Current	$\leq 0.01\% + 3\text{mA}$
Settings Resolution	Independent	Voltage	1mV
		Current	1mA
	Parallel	Voltage	1mV
		Current	1mA
	Series	Voltage	1mV
		Current	1mA
Read Back Resolution	Independent	Voltage	1mV
		Current	1mA
	Parallel	Voltage	1mV
		Current	1mA
	Series	Voltage	1mV
		Current	1mA
Settings Accuracy (Within 12 months) (25°C ± 5°C)	Independent	Voltage	$\pm(0.03\% \text{ of reading} + 10)\text{mV}$
		Current	$\pm(0.1\% \text{ of reading} + 5)\text{mA}$
	Parallel	Voltage	$\pm(0.03\% \text{ of reading} + 10)\text{mV}$
		Current	$\pm(0.2\% \text{ of reading} + 20)\text{mA}$
	Series	Voltage	$\pm(0.06\% \text{ of reading} + 20)\text{mV}$
		Current	$\pm(0.1\% \text{ of reading} + 5)\text{mA}$
Read Back Accuracy (25°C ± 5°C)	Independent	Voltage	$\pm(0.03\% \text{ of reading} + 10)\text{mV}$
		Current	$\pm(0.1\% \text{ of reading} + 5)\text{mA}$
	Parallel	Voltage	$\pm(0.03\% \text{ of reading} + 10)\text{mV}$
		Current	$\pm(0.2\% \text{ of reading} + 10)\text{mA}$
	Series	Voltage	$\pm(0.06\% \text{ of reading} + 20)\text{mV}$
		Current	$\pm(0.1\% \text{ of reading} + 5)\text{mA}$
Noise and Ripple (20Hz-20M)	Independent	Voltage(Vp-p)	$\leq 5\text{mVp-p}$
		Voltage(rms)	$\leq 1\text{mVrms}$
		Current(rms)	$\leq 5\text{mA rms}$

6. Technical Specification

Hz)	Parallel	Voltage(Vp-p)	≤5mVp-p
		Voltage(rms)	≤1mVrms
		Current(rms)	≤10mArms
	Series	Voltage(Vp-p)	≤10mVp-p
		Voltage(rms)	≤1mVrms
		Current(rms)	≤5mArms
Temperature Coefficient	Independent	Voltage	100ppm/°C
		Current	200ppm/°C
	Parallel	Voltage	100ppm/°C
		Current	200ppm/°C
	Series	Voltage	100ppm/°C
		Current	200ppm/°C
Programmable output		Storage	1M points
		Groups saved in internal memory	100 groups
		Time setting	Second
Remote Compensation Voltage (Two-wire)		≤1V	
Data Record Function		10k groups of data (voltage, current)	
Ports		USB Host, USB Device, RS232, LAN, supports USB TMC protocol	

ODP8354 Parameter

Parameter		Description	
Output Ratings (0°C-40°C)			CH1: 32V/5A, Maximum 102W constant power output CH2: 32V/5A, Maximum 102W constant power output CH3: 24V/3A, Maximum 24W constant power output CH4: 24V/3A, Maximum 24W constant power output
	Voltage/ Current		
	CH1,CH2 Parallel Voltage/ Current		64V/5A, Maximum 204W constant power output
	CH1,CH2 Series Voltage/ Current		32V/10A, Maximum 204W constant power output
Channel		4	
Load Regulation	Independent	Voltage	$\leq 0.01\% + 5\text{mV}$
	Parallel	Voltage	$\leq 0.01\% + 50\text{mV}$
	Series	Voltage	$\leq 0.01\% + 50\text{mV}$
Voltage Regulation	Independent	Voltage	$\leq 0.01\% + 3\text{mV}$
		Current	$\leq 0.01\% + 3\text{mA}$
	Parallel	Voltage	$\leq 0.01\% + 3\text{mV}$
		Current	$\leq 0.01\% + 3\text{mA}$
	Series	Voltage	$\leq 0.01\% + 3\text{mV}$

6. Technical Specification

		Current	$\leq 0.01\% + 3\text{mA}$
Settings Resolution	Independent	Voltage	1mV
		Current	1mA
	Parallel	Voltage	1mV
		Current	1mA
	Series	Voltage	1mV
		Current	1mA
Read Back Resolution	Independent	Voltage	1mV
		Current	1mA
	Parallel	Voltage	1mV
		Current	1mA
	Series	Voltage	1mV
		Current	1mA
Settings Accuracy (Within 12 months) (25°C ± 5°C)	Independent	Voltage	$\pm(0.03\% \text{ of reading} + 10)\text{mV}$
		Current	$\pm(0.1\% \text{ of reading} + 5)\text{mA}$
	Parallel	Voltage	$\pm(0.03\% \text{ of reading} + 10)\text{mV}$
		Current	$\pm(0.2\% \text{ of reading} + 20)\text{mA}$
	Series	Voltage	$\pm(0.06\% \text{ of reading} + 20)\text{mV}$
		Current	$\pm(0.1\% \text{ of reading} + 5)\text{mA}$
Read Back Accuracy (25°C ± 5°C)	Independent	Voltage	$\pm(0.03\% \text{ of reading} + 10)\text{mV}$
		Current	$\pm(0.1\% \text{ of reading} + 5)\text{mA}$
	Parallel	Voltage	$\pm(0.03\% \text{ of reading} + 10)\text{mV}$
		Current	$\pm(0.2\% \text{ of reading} + 10)\text{mA}$
	Series	Voltage	$\pm(0.06\% \text{ of reading} + 20)\text{mV}$
		Current	$\pm(0.1\% \text{ of reading} + 5)\text{mA}$
Noise and Ripple (20Hz-20MHz)	Independent	Voltage(Vp-p)	$\leq 5\text{mVp-p}$
		Voltage(rms)	$\leq 1\text{mVrms}$
		Current(rms)	$\leq 5\text{mA rms}$
	Parallel	Voltage(Vp-p)	$\leq 5\text{mVp-p}$

6. Technical Specification

		Voltage(rms)	≤1mVrms
		Current(rms)	≤10mArms
	Series	Voltage(Vp-p)	≤10mVp-p
		Voltage(rms)	≤1mVrms
		Current(rms)	≤5mArms
Temperature Coefficient	Independent	Voltage	100ppm/°C
		Current	200ppm/°C
	Parallel	Voltage	100ppm/°C
		Current	200ppm/°C
	Series	Voltage	100ppm/°C
		Current	200ppm/°C
Programmable output		Storage	1M points
		Groups saved in internal memory	100 groups
		Time setting	Second
Remote Compensation Voltage (Two-wire)		≤1V	
Data Record Function		10k groups of data (voltage, current)	
Ports		USB Host, USB Device, RS232, LAN, Support USB TMC	

General Parameter

Display

Characteristics	Description
Display Type	4.3 inch colored LCD (Liquid Crystal Display)
Display Resolution	480 (Horizontal) × 3(RGB) × 272 (Vertical) Pixels
Display Colors	16.7M colors, IPS

6. Technical Specification

Power Supply

Characteristics	Description		
Supply	110 VAC $\pm$ 10% or 220 VAC $\pm$ 10%; AC input 50/60Hz		
Fuse	ODP8353	110 V	250 V, F5A
		220 V	250 V, F3A
	ODP8354	110 V	250 V, F5A
		220 V	250 V, F3A

Environment

Characteristics	Description
Temperature	Working temperature: 0°C ~ 40°C Storage temperature: -20°C ~ 60°C
Relative Humidity	$\leq$ 90%
Height	Operating: 3,000 m Non-operating: 15,000 m
Cooling Method	Fan cooling

Mechanical Specifications

Characteristics	Description	
Dimension	212mm(W)*130mm(H)*290mm(D)	
Weight	ODP8353	Approx. 9 kg
	ODP8354	Approx. 9 kg

Interval Period of Adjustment:

One year is recommended for the calibration interval period.

7. Appendix

7.1 Appendix A: Packaging

(The accessories subject to final delivery.)

Standard Accessories:



Power Cord



User Manual



USB Cable



Fuse

Options:



**Banana plug
to crocodile
clip test leads**

7.2 Appendix B: General Care and Cleaning

General Care

Do not store or leave the instrument where the liquid crystal display could be exposed to direct sunlight for long periods of time.

Caution: To avoid any damage to the instrument, do not exposed it to any sprays, liquids, or solvents.

Cleaning

Inspect the instrument as often as operating conditions require.

To clean the instrument exterior, perform the following steps:

1. Wipe the dust from the instrument surface with a soft cloth. Take care not to scratch the transparent LCD protection screen when cleaning.
2. Disconnect power before cleaning your instrument. Clean the instrument with a damp soft cloth (not dripping with water). It is recommended to clean with soft detergent or fresh water. To avoid damage to the instrument, do not use any corrosive chemical cleaning agents.



Warning: Before re applying power, ensure that the instrument is completely dry, avoiding any electric shock or electrical short circuit resulting from moisture.
